


TruSeq Custom Amplicon Kit Dx[®]

Workflow and Kit Tracking Form FOR *IN VITRO* DIAGNOSTIC USE

For detailed instructions, refer to the *TruSeq Custom Amplicon Kit Dx Package Insert (document # 1000000029772)*.

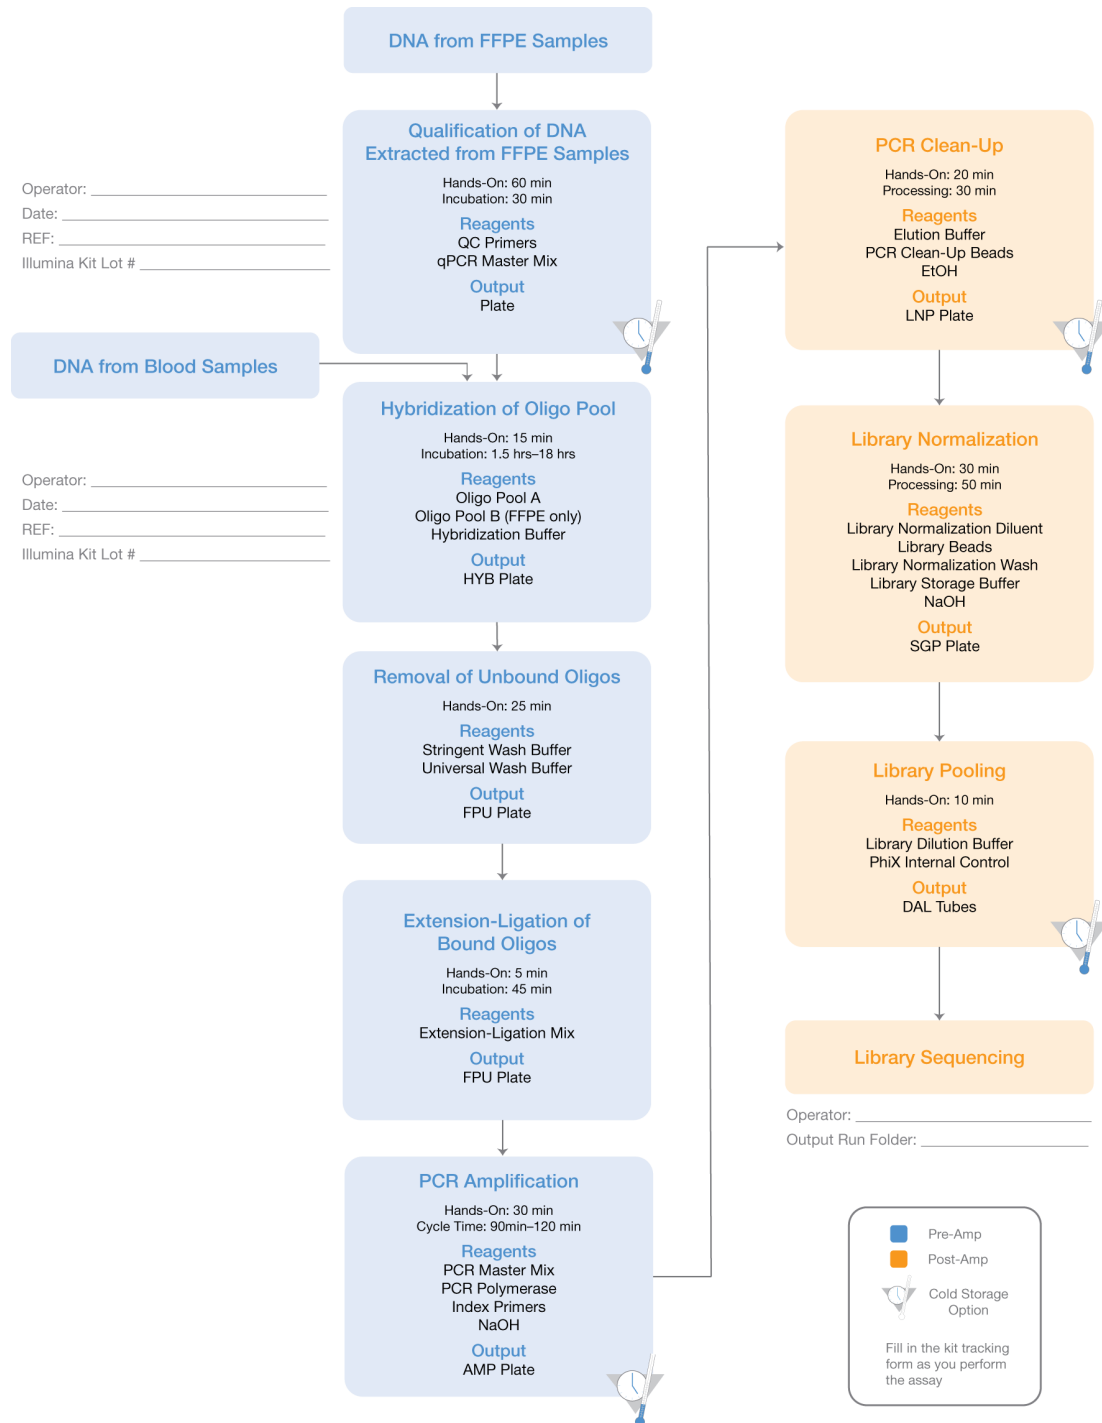

TruSeq Custom Amplicon Kit Dx


Workflow and Kit Tracking Form

[This page intentionally left blank]



Illumina
5200 Illumina Way
San Diego, California 92122 U.S.A.
+1.800.809.ILMN (4566)
+1.858.202.4566 (outside North America)
techsupport@illumina.com
www.illumina.com

Document # 1000000039154 v01
Page 2 of 2



Illumina Netherlands B. V.
Freddy van Riemsdijkweg 15
5657 EE Eindhoven
The Netherlands



Australian Sponsor:
Illumina Australia Pty Ltd
Nursing Association Building
Level 3, 535 Elizabeth Street
Melbourne, VIC 3000
Australia